

ROOM PLAN LOCATED ON PAGE 6-12


ITEM	QUANTITY	ITEM DESCRIPTION	WEIGHT	HEAT OUTPUT
①	1	CT HiSpeed ADVANTAGE GANTRY	3700 lb 1681 kg	24400 btu 7150 W < TYP> 29190 btu 8556 W < MAX>
②	1	PATIENT TABLE WITH EXTENDED TABLE TOP.	1185 lb 539 kg	700 btu 200 W
③	1	OPERATOR'S / PHYSICIAN'S CONSOLE	270 lb 123 kg	2400 btu 700 W
④	1	POWER DISTRIBUTION UNIT	1088 lb 495 kg	3400 btu 1000 W
⑤	1	MAIN COMPUTER CABINET	250 lb 114 kg	5450 btu 1600 W
⑥	1	SCAN UNIT CABINET	500 lb 227 kg	3400 btu 1000 W
⑦	1	INDEPENDENT CONSOLE	270 lb 122 kg	2400 btu 700 W
⑧	1	OPERATOR'S CHAIR		
⑨	1	INDEPENDENT CONSOLE COMPUTER	250 lb 114 kg	5462 btu 1600 W
⑩	1	LASER IMAGER SYSTEM	686 lb 312 kg	2220 btu 651 W
***** CUSTOMER/CONTRACTOR SUPPLIED AND INSTALLED ITEMS *****				
60		CLOSED CIRCUIT TV CAMERA		
61		CLOSED CIRCUIT TV MONITOR		

ENVIRONMENT


Ambient Operation Temperature: 55-75° (F)
 Allowable Temperature Change: 15° (F) per hour
 Humidity: 20-80 percent non condensing
 Allowable Humidity Change: 10 percent per hour
 Max - Altitude: 8000 ft. above sea level



CT HiSpeed ADVANTAGE

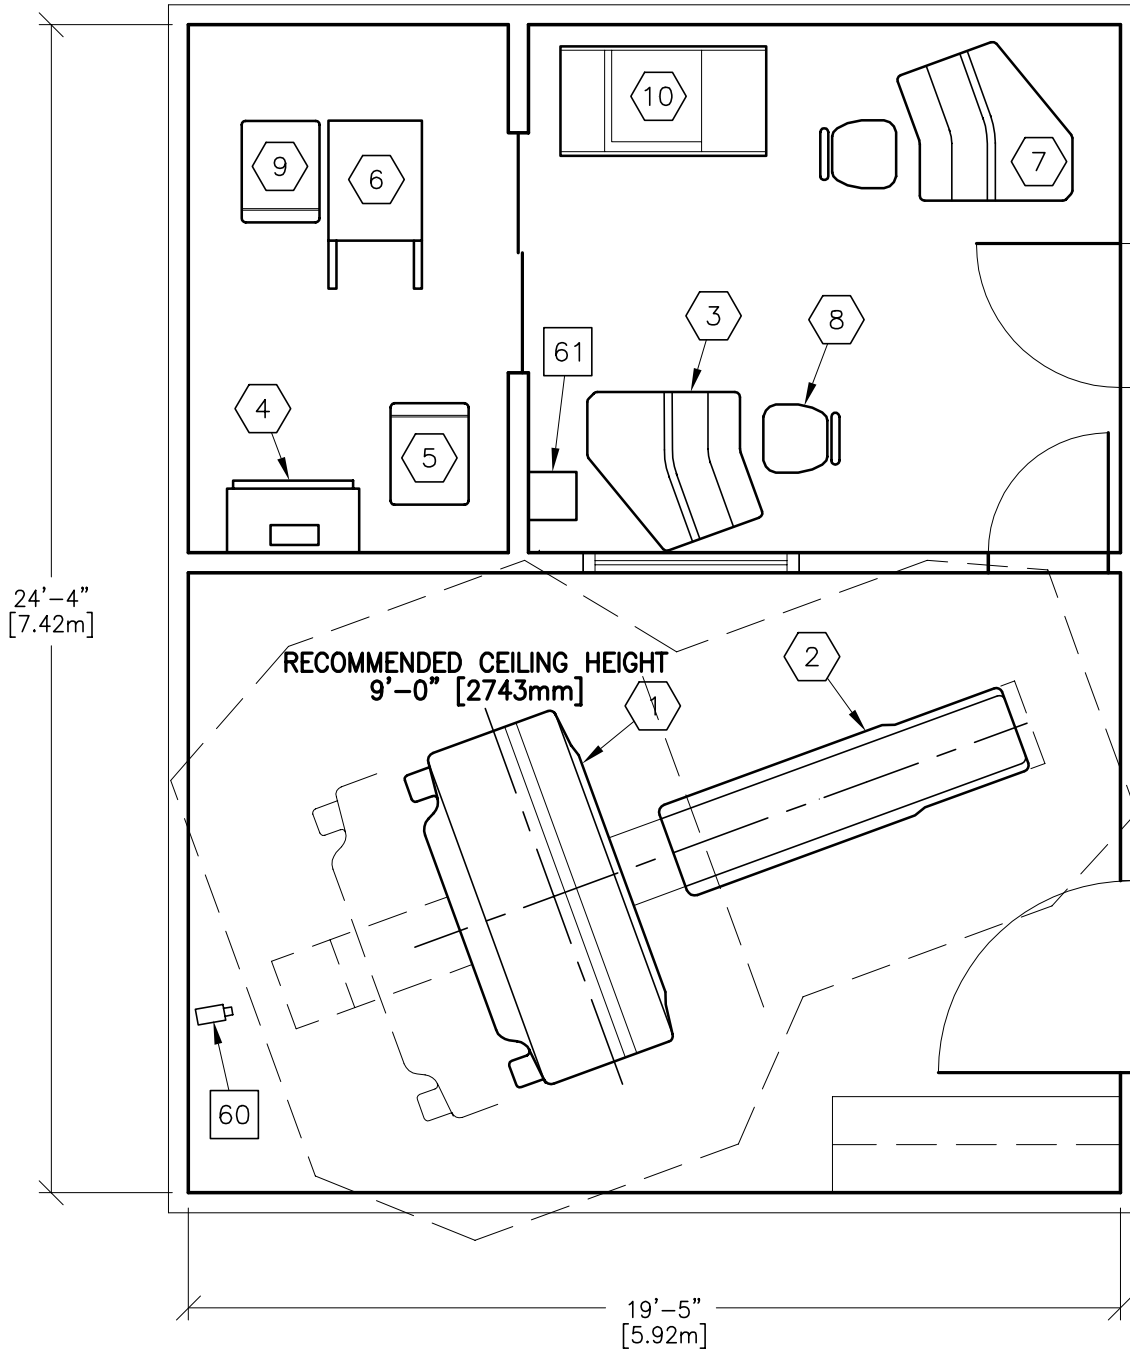

ROOM DIMENSIONS	LENGTH & WIDTH	CEILING HEIGHT
MINIMUM:	24'-0" x 19'-0" [7.31m x 5.79m]	9'-0" [2.74m]



SEE APPENDIX "A" FOR POWER SPECIFICATIONS